

Fig. 2a



Fig. 2b

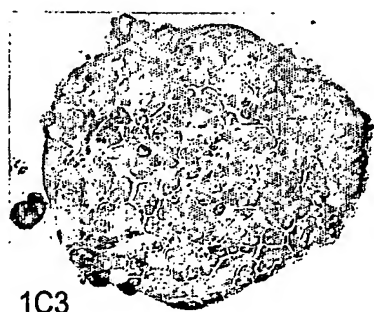


Fig. 2c

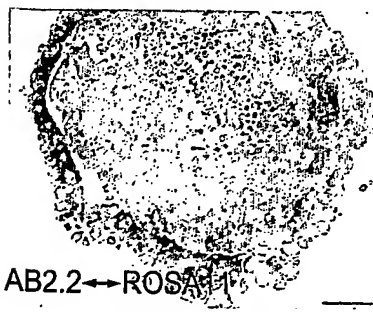


Fig. 2d

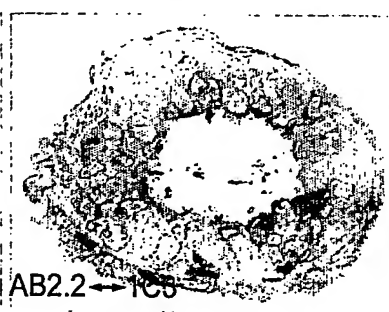


Fig. 2e

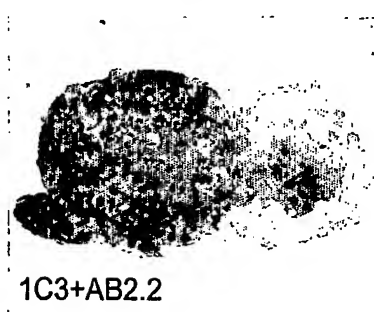


Fig. 2f

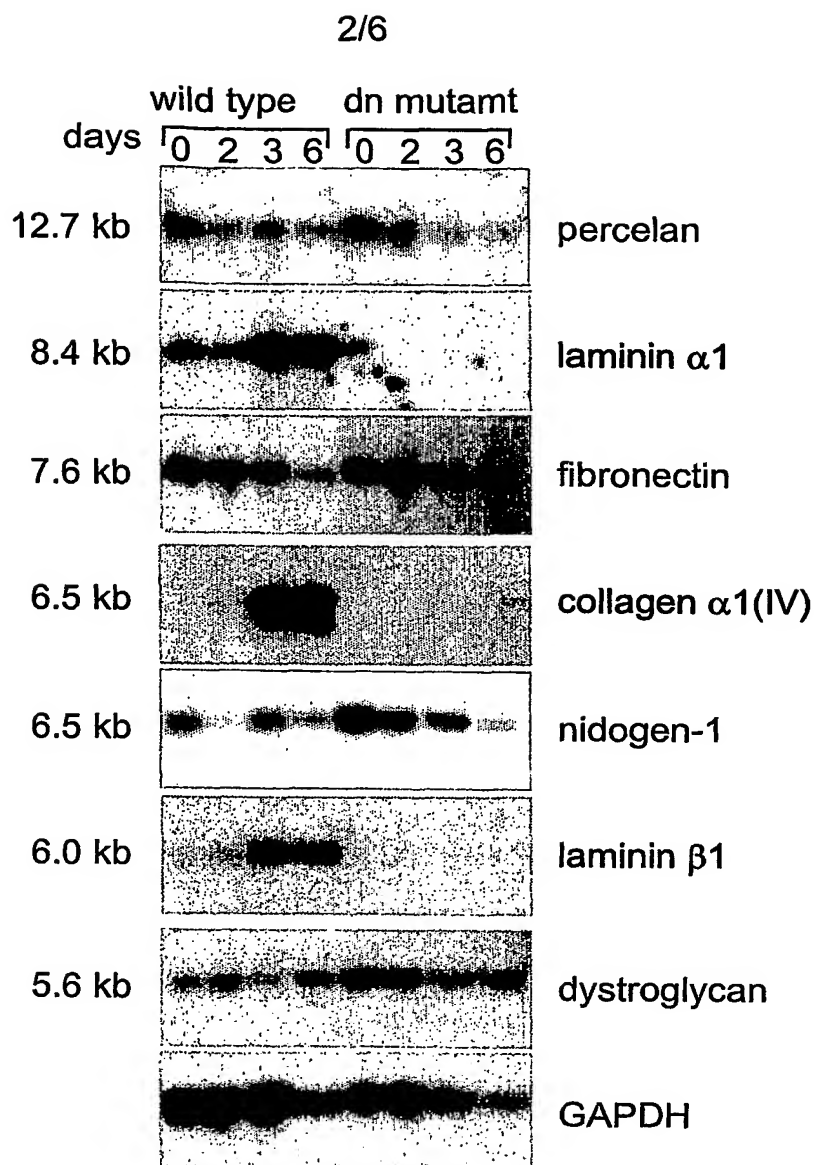


Fig. 3



Fig. 4

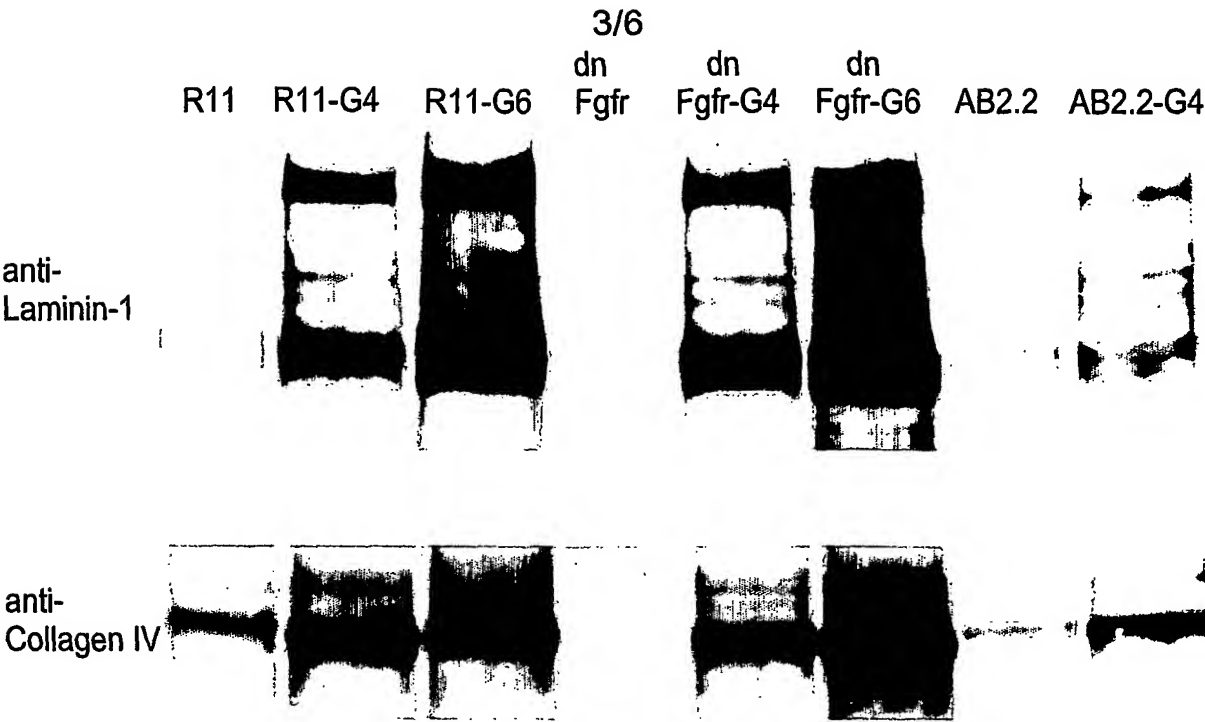


Fig. 5



Fig. 6a

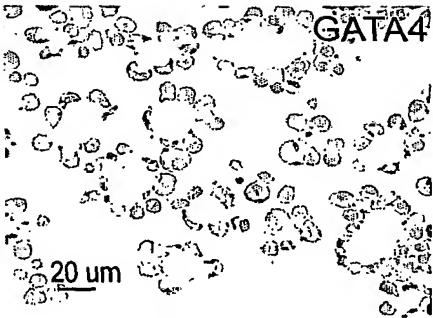


Fig. 6a

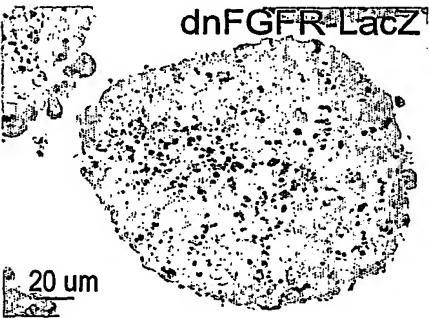


Fig. 6c

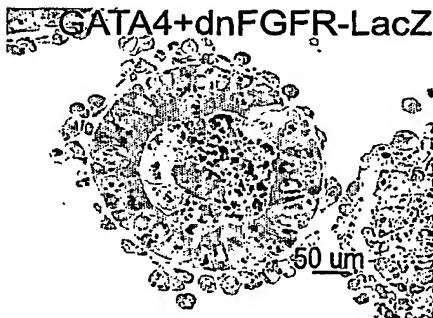


Fig. 6d

4/6

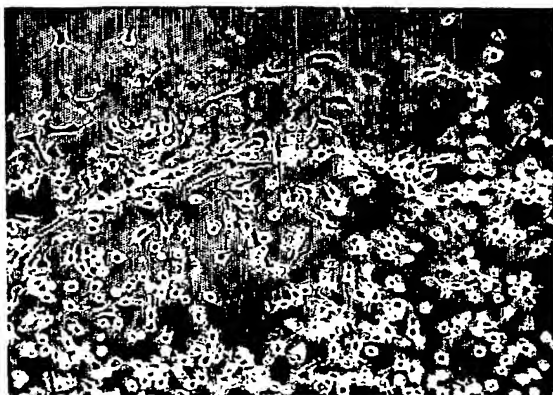


Fig. 7a



Fig. 7b

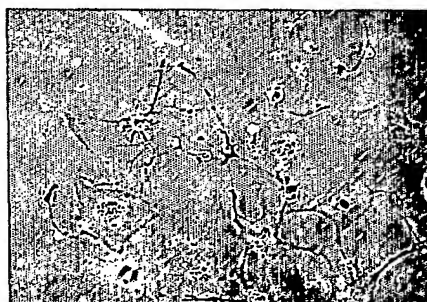


Fig. 8a



Fig. 8b

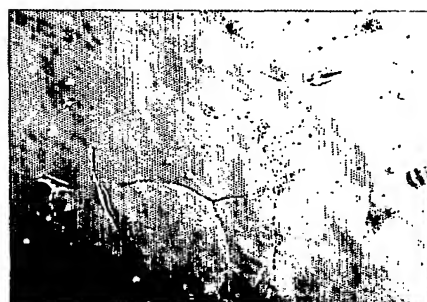


Fig. 8c



Fig. 8d

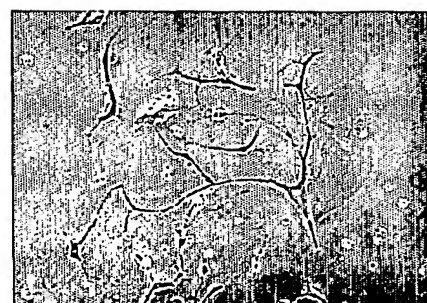


Fig. 8e



Fig. 8f

5/6

Tub III

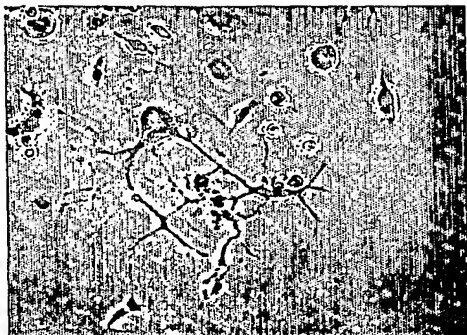


Fig. 9a



Fig. 9b

S100



Fig. 9c

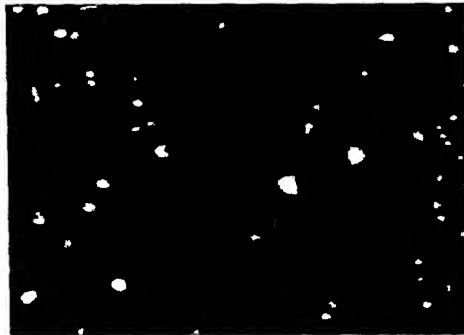


Fig. 9d

NSE



Fig. 9e



Fig. 9f

6/6

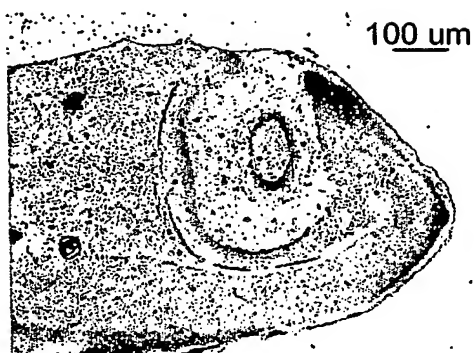


Fig. 10a

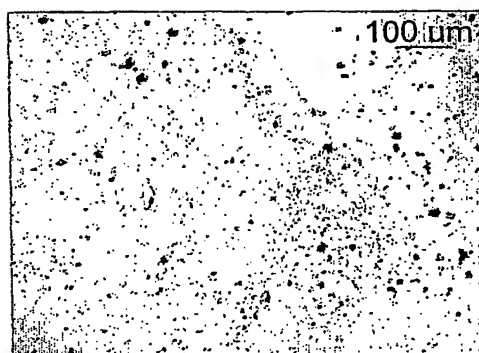


Fig. 10b

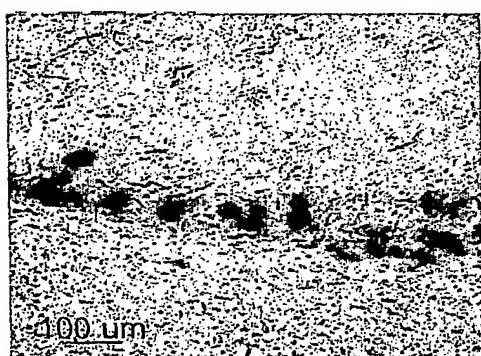


Fig. 10c

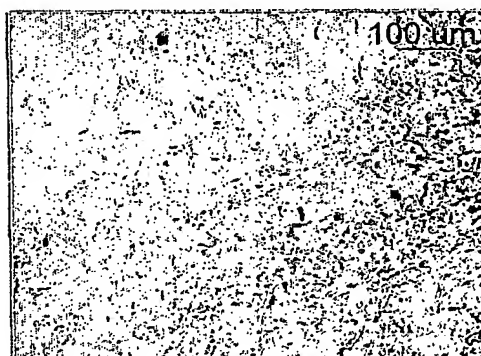


Fig. 10d



Fig. 11a



Fig. 11b



Fig. 11c